


Calibration Using 15L or 17L Cylinders

ITEMS REQUIRED TO CALIBRATE A STANDARD GAS DETECTOR USING A 15L OR 17L CYLINDER OF GAS:

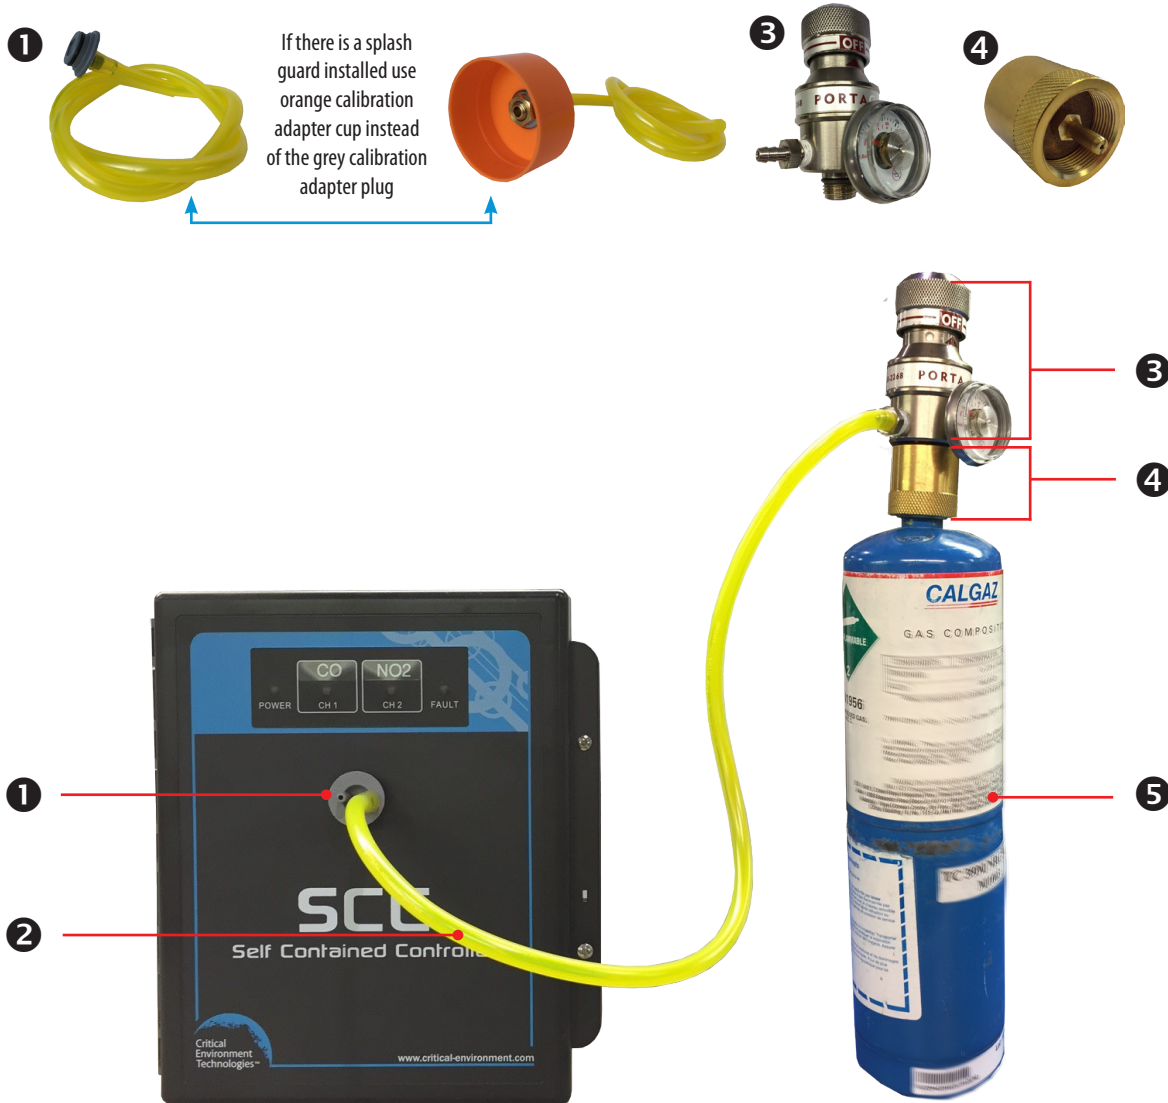

| NUMBER | FUNCTION | PART NUMBER |
|--------|--|------------------------------|
| 1 | Grey calibration adapter plug with o-ring and two zeroing port nozzles. Fits industry standard internal sensor vent openings. Comes with tubing attached (see 2) Orange calibration adapter cup for splash guard. Comes with tubing attached. | CET-7000-CAP CET-4700-SCC |
| 2 | Standard tubing (approx 61 cm / 2 ft long) included and attached to calibration adapter plug | n/a |
| 3 | Regulator for fixed flow @0.5 LPM. Fits 34 L, 58 L, 74 L, and 103 L cylinders | REG-0715-CR2 |
| 4 | Brass fitting to convert fixed flow regulator to attach to 15L and 17 L gas cylinders | REG-ADAPTER |
| 5 | Span Gas / Zero Gas cylinder, with air balance or nitrogen balance (electrochemical sensors), with air balance only (catalytic sensors) | various |